


Installation of CoAnn microSPE trap column and integrated analytical column in a nanoLC system

Installation of fitted trap (microSPE) column

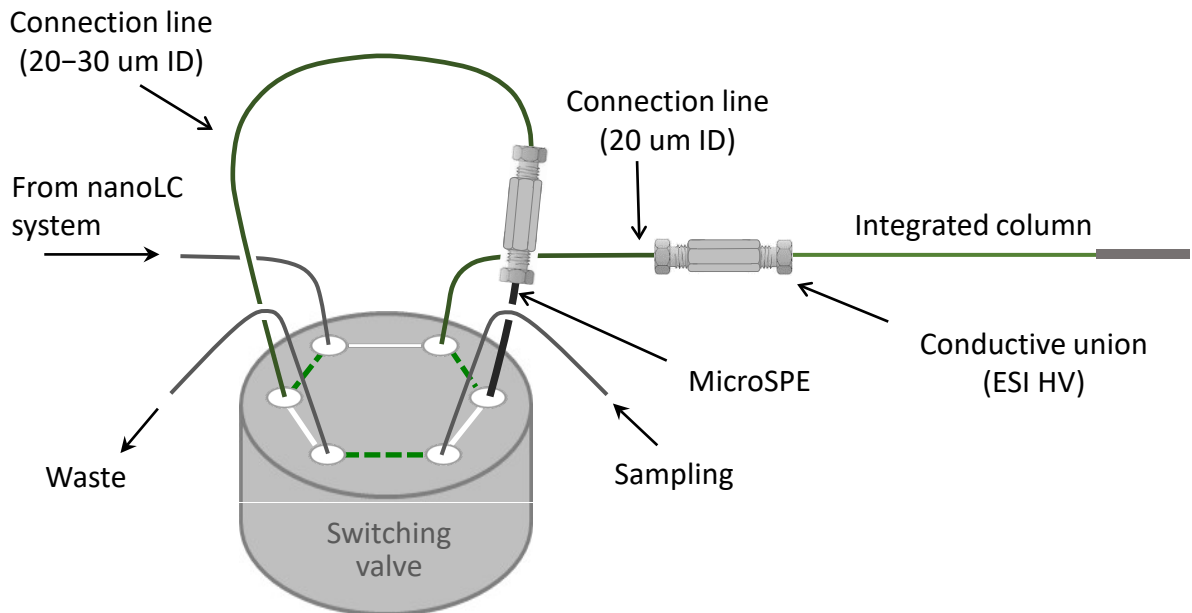

Installation of bare (unfitted) trap (microSPE) column (360 um OD)

A bare microSPE column (360 um OD) can be connected to a nanoLC column and nanoLC system via a VICI or IDEX 360 um fingertight union (for manual operation, as shown for USB column), or a nanoLC system with the switching valve 1/16" output port to 360 um via a VICI 1/16"-360 reducer (for automatic operation).